

CELL-DYN 29 Plus Control (with Retic)



CONTROL L N H


Refer to the appropriate system operator's manual for proper use of CELL-DYN Calibrator and Control Products.

IMPORTANT: Mixing and Handling


1. Remove a vial of the control from the refrigerator and warm to room temperature (18° to 30° C) for 15 minutes before use.
2. To mix: **(Do NOT mix mechanically or vortex.)**

For a video demonstration, visit www.corelaboratory.abbott and navigate to the Customer Portal → Technical Library → Other Reference Documents → Hematology Aids.

- a. Hold the vial vertically and roll each vial between the palms of the hands for 15-20 seconds.



- b. Continue to mix by holding the vial by the ends between the thumb and finger, rapidly inverting the vial 20 times end-over-end using a very quick turning motion of the wrist.

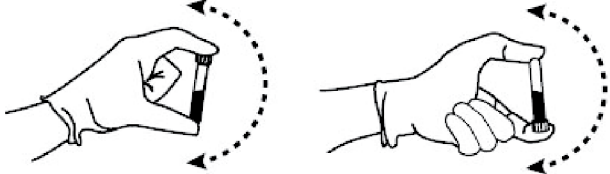

- c. Analyze immediately after mixing. Subsequent analyses during this test period may be performed by inverting the vial 5 times prior to instrument analysis.
- d. Steps a-c must be repeated upon removing the sample from the refrigerator for the entire open-vial time period regardless of the method of analysis (open tube, cap piercing, auto sample or manual sample).

3. Refer to the appropriate CELL-DYN System Operator's Manual for information about analyzing control specimens.

NOTE: For CELL-DYN Ruby:

- Perform stain of CELL-DYN 29 Plus Control (with Retic) as a patient sample as described in the CELL-DYN Ruby Reticulocyte Reagent package insert, except limit the staining time to between 15 and 30 minutes.

4. FOR AUTOMATED SAMPLING OR MANUAL CLOSED SAMPLING (CS):

- Refer to the appropriate CELL-DYN Operator's Manual. Remove the vial from the sample handler immediately after sampling.

FOR OPEN-VIAL SAMPLING:

- Aspirate a sample from the vial.
- Carefully wipe the vial rim and cap with a lint-free tissue.
- Replace the cap, ensuring it is on tight.

After sampling, return vial to refrigerator for maximum open-vial stability. If run in the open mode, wipe the threads of both vial and cap before replacing cap and returning to refrigerator.

Exp. 2026-04-03	7 Consecutive Day Open-Vial Stability
-----------------	---------------------------------------

Exp. 2026-04-03	7 Consecutive Day Open-Vial Stability
-----------------	---------------------------------------

SYSTEM	CONTROL L		CONTROL N		CONTROL H	
CELL-DYN Sapphire	LOT L60199		LOT N60199		LOT H60199	
PARAMETER	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **
WBC 10 ⁹ /L	2.95	0.40	6.77	0.80	15.9	3.0
NEU 10 ⁹ /L	1.66	0.20	4.10	0.40	10.4	1.1
NEU %	56.2	6.0	60.5	5.0	65.5	6.0
LYM 10 ⁹ /L	0.86	0.20	1.71	0.50	3.21	1.00
LYM %	29.0	8.0	25.3	6.0	20.2	5.0
MONO 10 ⁹ /L	0.34	0.20	0.76	0.40	1.80	0.60
MONO %	11.4	6.0	11.2	5.0	11.3	3.0
EOS 10 ⁹ /L	0.10	0.10	0.18	0.17	0.43	0.19
EOS %	3.00	3.00	2.65	2.00	2.69	1.00
BASO 10 ⁹ /L	0.10	0.10	0.25	0.25	0.50	0.50
BASO %	1.50	1.50	1.50	1.50	1.50	1.50
RBC 10 ¹² /L	2.87	0.18	4.22	0.20	5.17	0.30
RBC _{co} 10 ¹² /L	2.96	0.18	4.26	0.20	5.16	0.30
HGB g/dL	7.83	0.30	12.0	0.5	16.3	0.8
HCT %	22.4	1.5	33.8	2.5	45.3	3.0
MCV fL	77.9	4.0	80.2	4.0	87.6	4.0
MCH pg	27.3	2.0	28.4	2.0	31.5	2.0
MCHC g/dL	35.0	2.3	35.5	2.3	36.0	2.3
RDW %	15.0	2.5	15.0	2.5	14.5	2.5
NRBC 10 ⁹ /L*	0.001	0.001	0.001	0.001	2.18	0.60
NRBC/100WBC*	0.001	0.001	0.001	0.001	13.7	2.5
PLT 10 ⁹ /L	69.4	20.0	209	50	444	60
PLT _i 10 ⁹ /L	75.4	20.0	227	50	468	60
MPV fL	9.38	2.00	8.21	2.00	7.86	2.00
RET _C 10 ⁹ /L	230	50	144	50	97.7	50.0
%R	8.00	1.50	3.40	1.00	1.89	0.80
IRF	0.54	0.18	0.46	0.14	0.42	0.10

SYSTEM	CONTROL L		CONTROL N		CONTROL H	
CELL-DYN Ruby	LOT L60199		LOT N60199		LOT H60199	
PARAMETER	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **
WOC 10 ⁹ /L	3.1	0.4	7.1	0.7	16.5	2.5
NOC 10 ⁹ /L	3.1	0.4	7.1	1.0	18.7	2.5
NEU 10 ⁹ /L	1.8	0.3	4.4	0.8	10.9	2.0
NEU %	57.1	6.0	61.5	6.0	65.9	10.0
LYM 10 ⁹ /L	0.9	0.3	1.7	0.8	3.1	2.0
LYM %	27.7	7.0	23.5	6.0	19.0	10.0
MONO 10 ⁹ /L	0.3	0.2	0.7	0.4	1.7	0.6
MONO %	9.0	5.0	9.6	4.5	10.1	3.0
EOS 10 ⁹ /L	0.1	0.1	0.2	0.2	0.5	0.2
EOS %	3.0	3.0	2.5	2.0	2.8	1.0
BASO 10 ⁹ /L	0.1	0.1	0.2	0.2	0.6	0.6
BASO %	3.7	3.0	3.0	3.0	3.0	3.0
RBC 10 ¹² /L	2.90	0.15	4.29	0.20	5.32	0.28
HGB g/dL	7.7	0.4	11.9	0.5	16.8	0.6
HCT %	21.5	1.5	32.9	2.3	44.0	3.5
MCV fL	74.2	4.0	76.6	4.0	82.8	4.0
MCH pg	26.6	2.0	27.7	2.0	31.6	2.0
MCHC g/dL	35.8	2.3	36.2	3.0	38.2	2.3
RDW %	12.9	2.5	12.6	2.5	11.1	2.5
PLT 10 ⁹ /L	71	20	225	30	493	60
MPV fL	6.4	2.0	6.2	2.0	6.1	2.0
Retic %***	5.1	1.5	1.9	1.0	1.1	0.8

Exp. 2026-04-03	7 Consecutive Day Open-Vial Stability
-----------------	---------------------------------------

SYSTEM	CONTROL L		CONTROL N		CONTROL H	
Manual Count ¹	LOT L60199		LOT N60199		LOT H60199	
PARAMETER	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **	ASSAY VALUE	± MEAN RANGE **
Retic %	5.2	2.0	2.4	1.5	0.8	0.8

NOTE: Flags may occur with control materials. PIC/POC alarms may be seen with this control when used on the CELL-DYN Sapphire. The alarms may be disregarded if the control is performing within the assay ranges.

* NOTE: The Assay Value of .001 and Mean Range of ± .001 for NRBC and NRBC/100WBC is entered for the Level L and Level N controls since the instrument will not accept a value of zero. The NRBC concentration for Levels L and N is below the detectable level of the instrument and as such serves as the NRBC negative control. The Level H is the NRBC positive control.

** The mean range does not represent standard deviations (SD).

*** Retic % values for CELL-DYN Ruby are included as separate files.

¹ Manual values were obtained using the Miller Ocular method.



CELL-DYN, CELL-DYN Sapphire and CELL-DYN Ruby are trademarks of Abbott Laboratories in various jurisdictions.

Abbott Laboratories
Diagnostics Division
Abbott Park, IL 60064
USA

EC REP Abbott GmbH & Co. KG
Max-Planck-Ring 2
65205 Wiesbaden
Germany
+49-6122-580

MANUFACTURED FOR
Abbott Laboratories



REF 08H58-01, 08H58-02

